



weelko



HighTech Sauna Air WKB002

Pressotherapy + Thermotherapy

HighTech Sauna Air WKB002


Pressotherapy + Thermotherapy

Note: This instrument is delivered with a thin adhesive film protecting the touch screen against possible scratches that may occur during transport. This film can be removed after unpacking.

EQUIPMENT

- Pressotherapy right and left boot
- Right and left leg
- Abdomen
- Right and left arm
- Blanket and air tubes
- Main unit



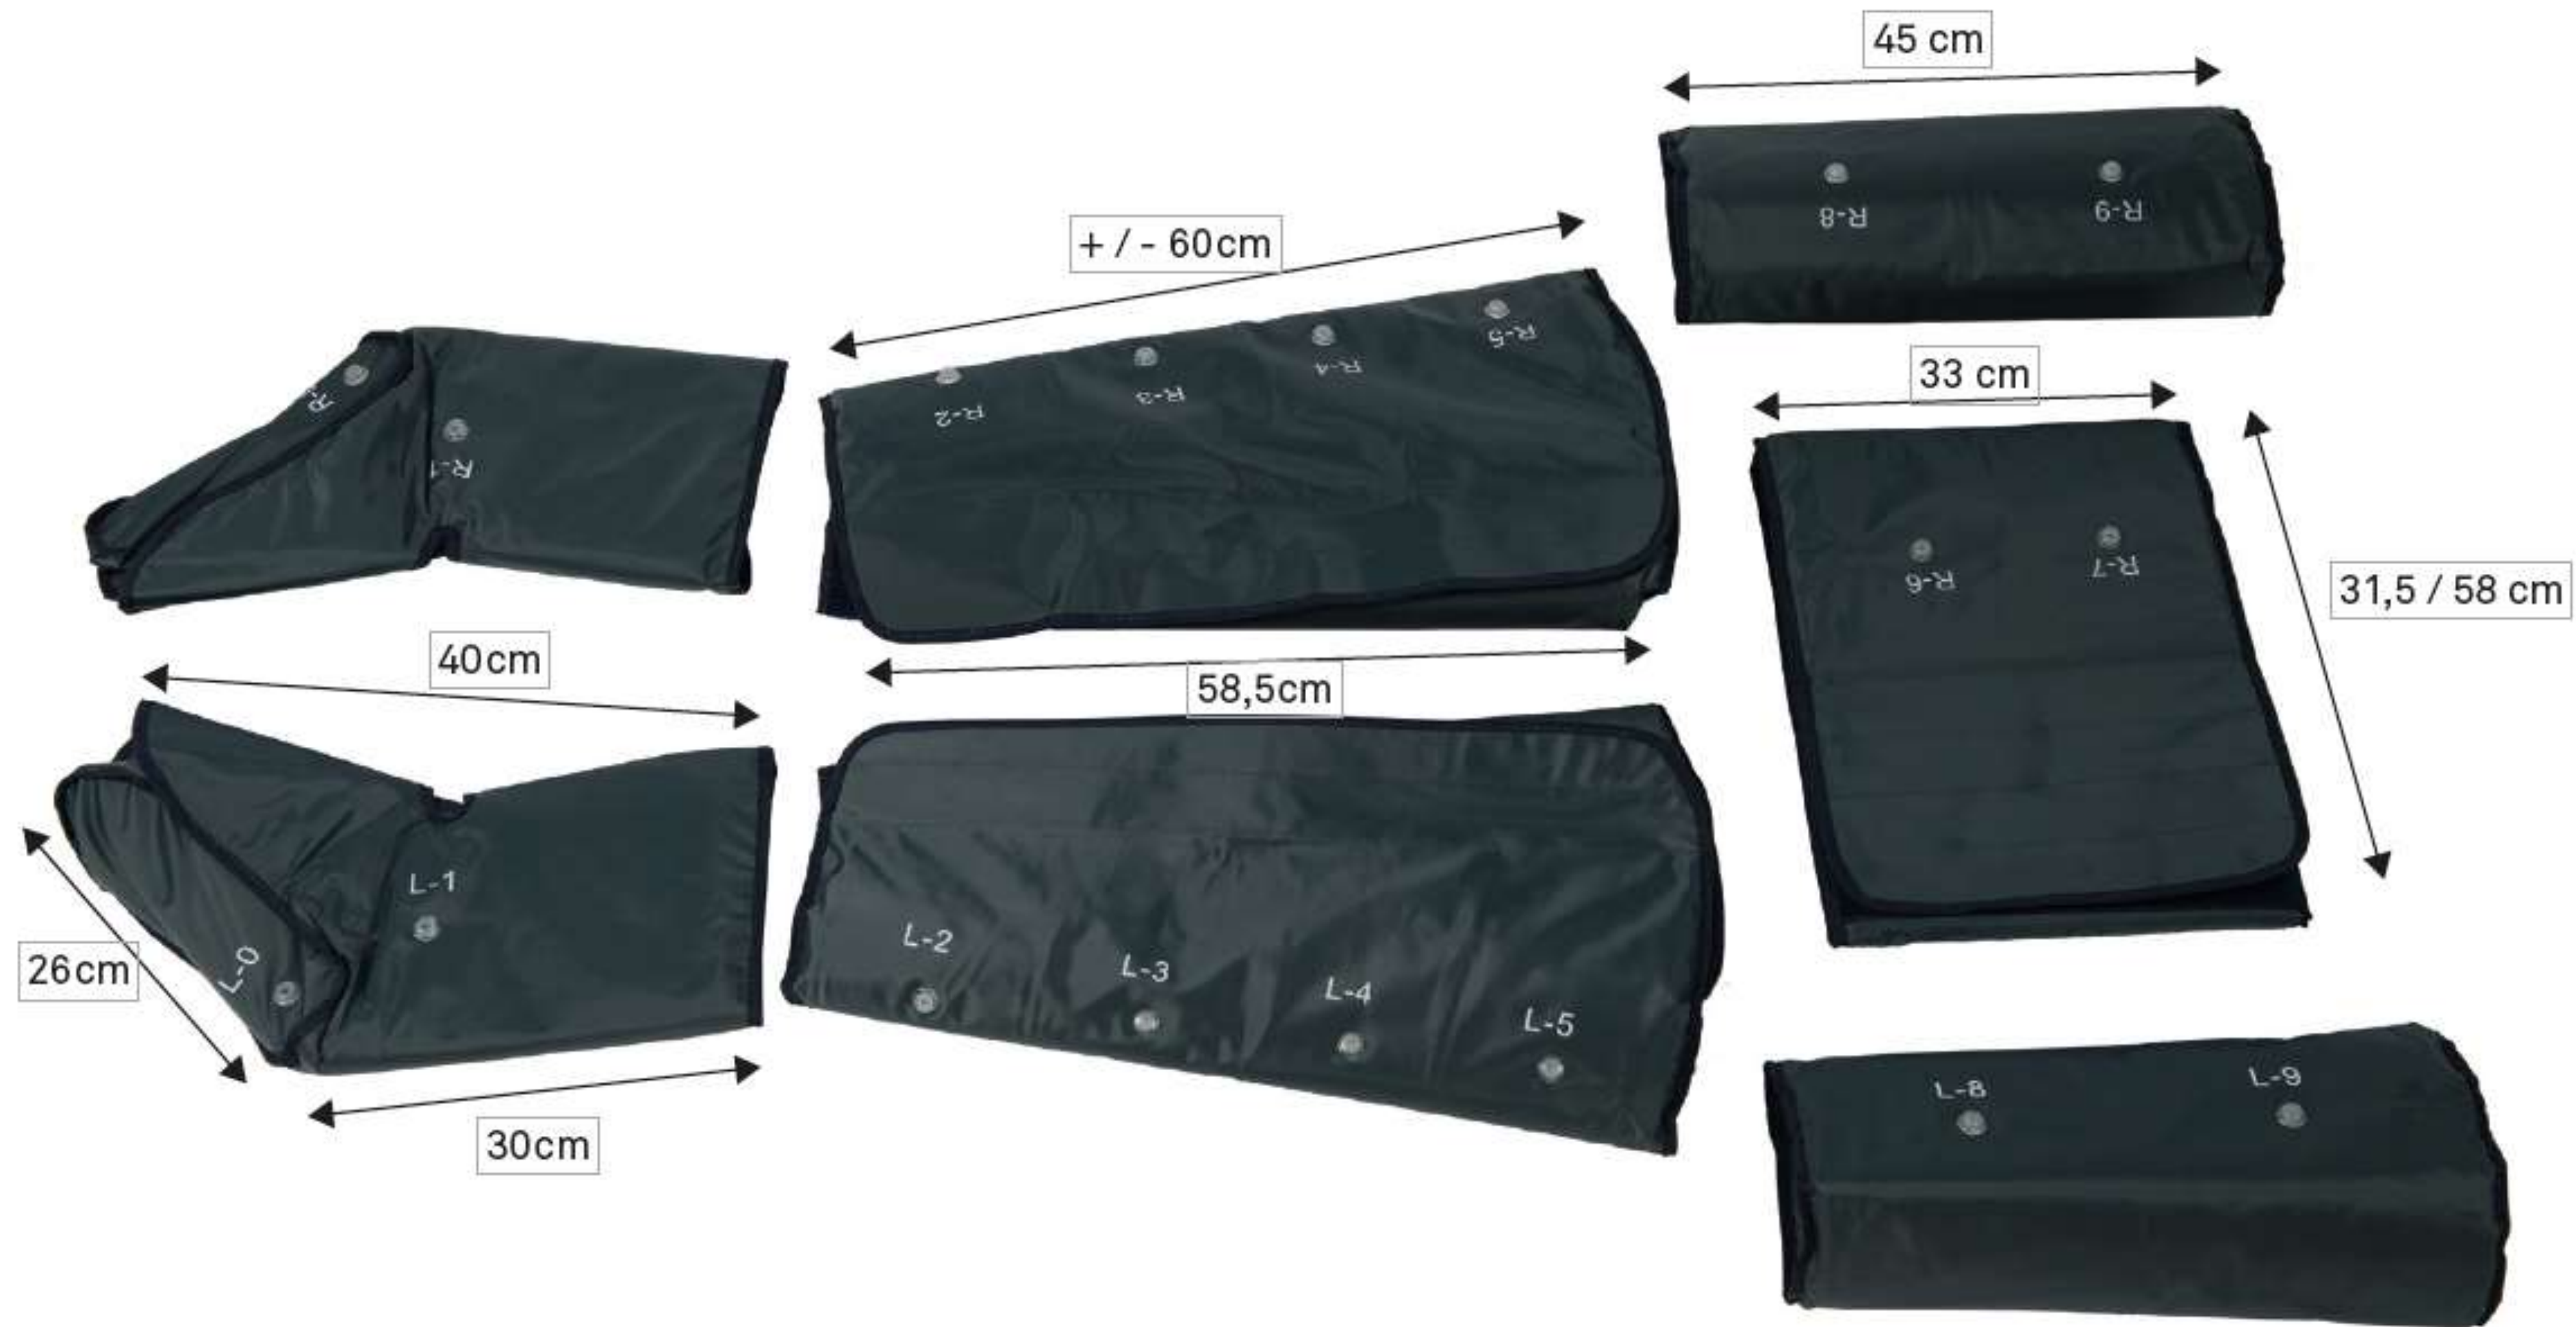

Our WKB002 is a digital instrument with touch screen which combines two functions: thermotherapy and pressotherapy.

Suit composed of boots, legs, abdomen and arms. It also includes a blanket to store the wires and the suit.

Ideal to improve circulation and to ease fat removal through the activation of the lymphatic drainage, the cellular oxygenation and muscle relaxation. It will be your major ally in body treatments.



HighTech Sauna Air WKB002

Pressotherapy + Thermotherapy

HighTech Sauna Air

WKB002

Pressotherapy + Thermotherapy

Connections are on the rear panel.
Connect as follows, from left to right:

- Plug in the power cable (200-240V 50Hz).
- Connect the tubes properly to the rear panel. Follow the numerical indications. Thin cables from 1 to 5 are for thermotherapy. Thick cables are for pressotherapy (3 connections).
- Place the blanket with the cables on a flat surface so that the customer can lay down on it. Cover the blanket with disposable paper to ensure the best hygienic conditions.
- Wrap the suit around the user's body and adjust it. Remember to use a disposable garment underneath the pressotherapy suit.





To switch on the device, press the button on the front panel and then click on the Weelko logo on the touch screen to select the desired menu. Choose “Pressotherapy”, for pressotherapy, or “Far infrared”, for thermotherapy.

Pressotherapy

Pressotherapy is a non-invasive and painless beauty treatment, which stimulates the lymphatic and circulatory systems. Its compression system is designed to increase the venous and lymphatic flow, improving venous return. Helps to remove toxins from the body and to revitalize and oxygenate the skin. Allows to achieve weight loss, to define the legs, abdomen and arms and to improve skin tone. The number of recommended sessions is 2-3 per week, but it can vary depending on the treatment and the results to achieve. Thus, a prior assessment of the customer is very important. This is a safe, relaxing and pleasant treatment. Hightech WKB002 is also equipped with thermotherapy, which is an excellent combination.

First, choose the treatment to perform:

Pressotherapy: to activate pressotherapy.

Far infrared: to activate thermotherapy.

Mode: as for pressotherapy, it allows to choose one of the four programs: A, B, C, D.

Level: to adjust the intensity of the treatment into 3 levels (low, medium and high), tailored to the client's needs. Always increase the intensity from less to more to prevent injury and check that the intensity is appropriate during the treatment.

Time: to specify the time of the treatment. Maximum recommended time is 30-45 min.

Play and Pause: to start or pause the device when necessary.



4 programs are provided:

Mode A fills with air sections from 0 to 9. Section 0 is deflated when section 1 is inflated. Section 1 is deflated when section 2 is inflated and so on from one limb to another, from toes to arms. The filling time per section is 11 seconds and there's a rest time of 11 seconds, which provides a pleasant feeling of light drainage. At the end of the program, sections from 0 to 9 are inflated at the same time and the program starts again.

Mode B fills with air sections from 0 to 9. Section 0 is deflated when section 2 is inflated. Section 1 is deflated when section 3 is inflated and so on from one side to another. The filling time is 11 seconds and the pressure is increased on all sections. At the end of the program, sections from 0 to 9 are inflated at the same time and the program starts again. The feeling of pressure is more intense and deep. Mode B is normally used to combat edematose cellulite, fat deposits and to prevent liquid retention.






Mode C fills with air sections from 0 to 9. First section 0 is inflated, then section 1, later section 2 and so on through all sections. The air pressure is not lost as in previous modes. There is a rest time of 11 seconds and, at the end, the program starts again from section 0. Mode C applies a stronger intensity, focusing on the abdomen and thighs. It is recommended for localized fat and more severe cellulite on thighs and abdomen.

Mode D fills with air the three sections at the same time: legs, abdomen and arms from bottom to top. This is a stronger mode, which focus on the abdomen and arms. It is recommended to prevent abdominal bloating and fluid retention in the arms.

If you don't want to use a concrete mode, the device allows to choose sections separately and to adjust the inflation intensity of each section. You just need to press the area you want to treat and adjust its intensity by using the buttons "+" and "-" from 0 to 15.

Mode of treatment

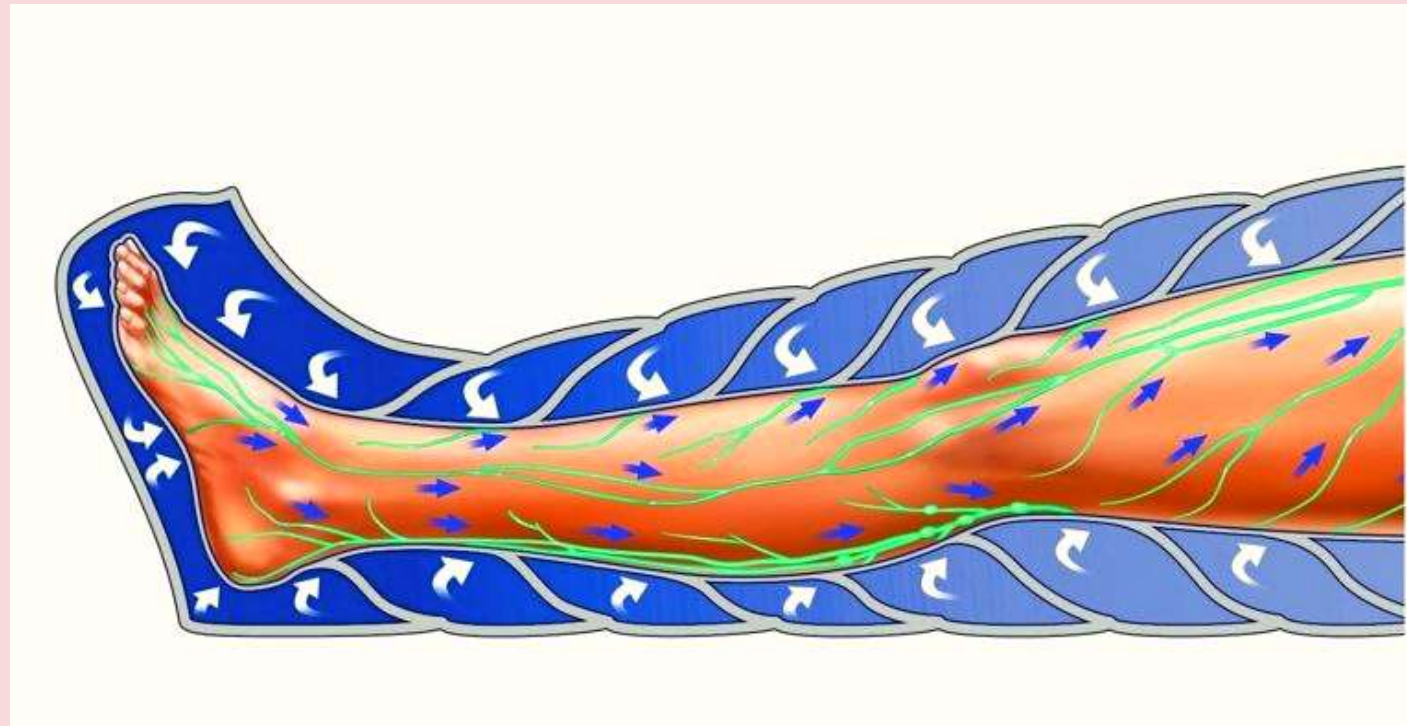

The application of air pressure, which stimulates the venous return, improves blood and lymph circulation. It has a thermal and calming effect on the body.

Place the customer in supine position on the treatment table and wrap the suit with the cables around the customer's body. During the treatment, adjust the pressure and time according to the customer's needs.

Thermotherapy

This device is also equipped with thermotherapy, which is the use of heat in therapy. It is indicated to activate blood circulation, to encourage fat metabolism, to relieve muscular pain or stiffness and it is also very relaxing. Body temperature will rise as the temperature of the equipment is increased (maximum operating temperature is 55°C). It has a therapeutic and relaxing effect on the body.

As the body is warmed, the blood circulation increases and the skin starts to sweat. Waste will be removed as the body tries to cool down.

It has 5 treatment zones, which allow to adjust the temperature separately, from 0°C to 62°C.

Application mode

- Connect the tubes properly to the rear panel. Follow the numerical instructions. Thin cables from 1 to 5 are for thermotherapy and thick cables from 0 to 9 are for pressotherapy.
- It is important to place the blanket on a flat surface so that the customer can lay down on it.
- Cover the blanket with disposable paper to ensure the best hygienic conditions.
- Wrap the suit around the user's body. Remember to use a disposable garment underneath the pressotherapy suit.
- Turn on the device, select the treatment to perform (pressotherapy or thermotherapy) and the intensity of the treatment.
- The pressure of the device is 20-40KPa, 25-40L/m.



Indications



- Treatments for fluid retention, swelling legs and lymphedema.
- Detox treatments (fat and toxins removal).
- Heavy legs treatments.
- Adjuvant in aesthetic treatments for removing localized fat.
- Helps to improve blood circulation in customers suffering from hypertension and diabetes.
- Helps to improve orange-peel skin appearance.
- Treatment and prevention of varicose veins.
- Stimulation of the circulatory system.
- Improves post-surgery lymph circulation.
- Muscle toning.
- Oxygenation of the body.

Contraindications

It is generally considered safe for adults of all ages, with few contraindications. However, it is important to consult a medical/aesthetic professional before getting any of these treatments.

- People with serious heart diseases.
- Phlebitis.
- Infectious diseases.
- Skin diseases and possible adverse reactions.
- People with weakened immune systems or cancer.
- Hormonal problems.
- Pregnant women can only get pressotherapy on legs and arms, with low pressure and only under medical prescription.
- Do not use on people with epilepsy, with a pacemaker or having a serious medical condition.
- It is not recommended to use on people with claustrophobia.

Precautions

- Be careful not to wrap the airbag too tight, to avoid hurting the users when the air is too strong. Always adjust the air pressure according to your customer's preferences.
- If the suit is broken or aged, please replace it with a new one to avoid accidental skin burns or electric shocks.
- During the session, check with the customer that the air pressure is appropriate.
- The customer is recommended to drink plenty of water before and after the treatment.
- Use a cellulose protector underneath the pressotherapy suit to ensure the best hygienic conditions.
- Do not let the suit heat without anyone inside.
- Do not expose the device to dripping or splashing.
- Be careful with the electric connections.
- This device should be assembled and disassembled by professional staff.
- In case of malfunction, check carefully all connections and contact your distributor.

Yubitzay Avila
Customer Training
T. +34 93 824 9020
y.avila@weelko.com
S. Yubitzay Avila

Weelko Barcelona S. L.
Pol. Ind. La Valldan
Camí de Garreta, 92
08600 Berga
Barcelona – Spain
T. +34 93 824 9020
info@weelko.com
www.weelko.com



Welcome to  weelko